


Total Volatile Organic Compound Measurement

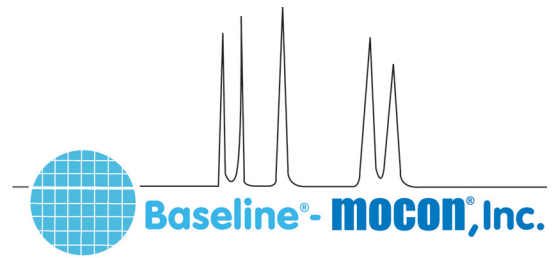

Sources of VOCs

Volatile Organic Compounds (VOCs) are potentially dangerous compounds created by both human industry and natural processes that vaporize under normal atmospheric conditions. VOC levels are much higher in indoor environments as they can be emitted by many manufactured products such as carpet, paint, and cleaning supplies. Outdoor sources can include landfills, industry, and hydrocarbon emissions.

Prolonged human exposure to VOCs have been known to cause respiratory problems, cancer, and neurological damage. Environmental damage can include air, water, and soil pollution.

Detection using a PID


Photoionization Detectors (PIDs) are the easiest and most efficient way to detect VOC levels. Although not as selective without the use of a gas chromatography column, a stand alone PID provides real time measurement of total volatile organic compounds in a portable format that anyone can use. These detectors enable the user to react swiftly to any potential threat, without waiting for the evaluation of a time-weighted average (TWA). Sensitivity can be increased by the selection of Ultra-violet (UV) lamp, as well as detector range.



Applications

- Industrial Hygiene & Safety Monitoring
- Confined Space Entry
- Soil Contamination & Remediation
- Hazmat Sites and Spills
- Arson Investigation
- Low Concentration Leak Detection
- EPA Method 21 and Emissions Monitoring
- Indoor Air Quality
- Homeland Security and Federal Customs
- Fenceline Monitoring
- Sick Building Syndrome
- Petrochemical Plants
- Electronics Manufacturing
- Paint Booths
- OSHA, NIOSH, EPA
- Construction Sites
- Waste Disposal
- Paper Manufacturing
- Agricultural Monitoring
- School Air Monitoring
- Military Operations
- Transportation Regulation

Total Volatile Organic Compound Measurement

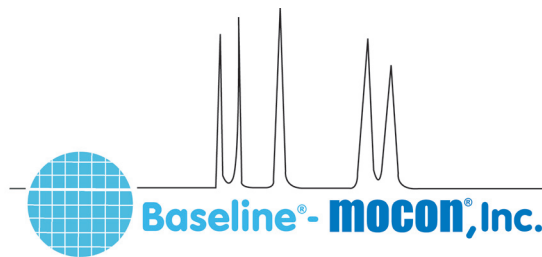

Ionization Potentials & Response Factors

The sample gas is exposed to an ultraviolet light from a lamp which ionizes the sample to be detected by the instrument and reported as a concentration. VOCs with an Ionization Potential (IP) less than the eV of the lamp will be detected by photoionization. The most common lamp is the 10.6 eV, although a 9.6 eV can also be used for increased selectivity.


The ratio between the sensitivity of Isobutylene to that of a target compound is called a Response Factor (RF). For example, the piD-TECH^{plus}® sensor has a typical sensitivity of 1mV/ppm for Isobutylene and 2mV/ppm for Benzene. That means that Benzene's RF is equal to 0.5.

The RF allows the user to measure the concentration of various gases without actually calibrating the sensor with the target gas. A comprehensive list of Ionization potentials and Response Factors is available from Baseline-MOCON at request.

Common VOCs

Chemical	Source	IP	RF
Acetone	Solvent	9.7	1.2
Arsine	Electrical Manufacturing	9.9	2.6
Butadiene	Rubber / Elastomers	9.1	0.69
Benzene	Petroleum / Polymer	9.3	0.53
Cumene	Petroleum / Polymer	8.8	0.54
Dimethoxymethane	Solvent	10	11.3
Ethyl Mercaptan	Natural Gas	9.3	0.6
Hydrogen Sulfide	Natural Gas	10.5	3.2
Mesityl Oxide	Manufacturing By-product	9.1	0.47
Methyl Ethyl Ketone	Solvent	9.5	0.9
Methyl Mercaptan	Natural Gas	9.4	0.6
Nitric Oxide	Manufacturing By-product	9.3	7.2
Phosphine	Electrical Manufacturing	9.87	2.8
Styrene	Petroleum / Polymer	8.5	0.4
Toluene	Petroleum / Polymer	8.8	0.53
Vinyl Chloride	Manufacturing By-product	10	1.8

Linearity

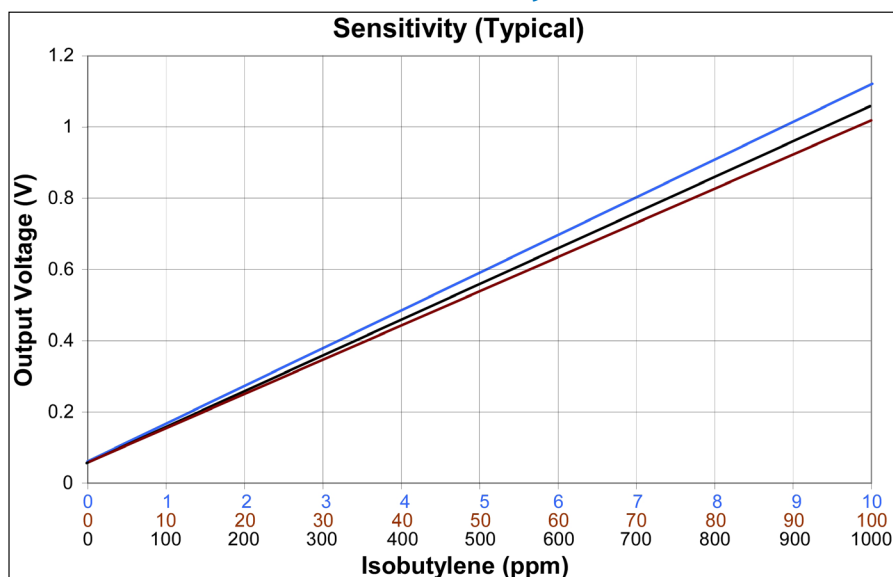

A022.1

P.O. Box 649, 19661 Highway 36 • Lyons, CO 80540

P: 1.800.321.4665 • 1.303.823.6661 F: 303.823.5151 E: Sales@BaselineIndustries.com