



Note: Regulator (shown in circle) can be fitted here or supplied loose issue for installation by others close to the sample take off point.

Sample must be clean i.e. particulate and aerosol free.

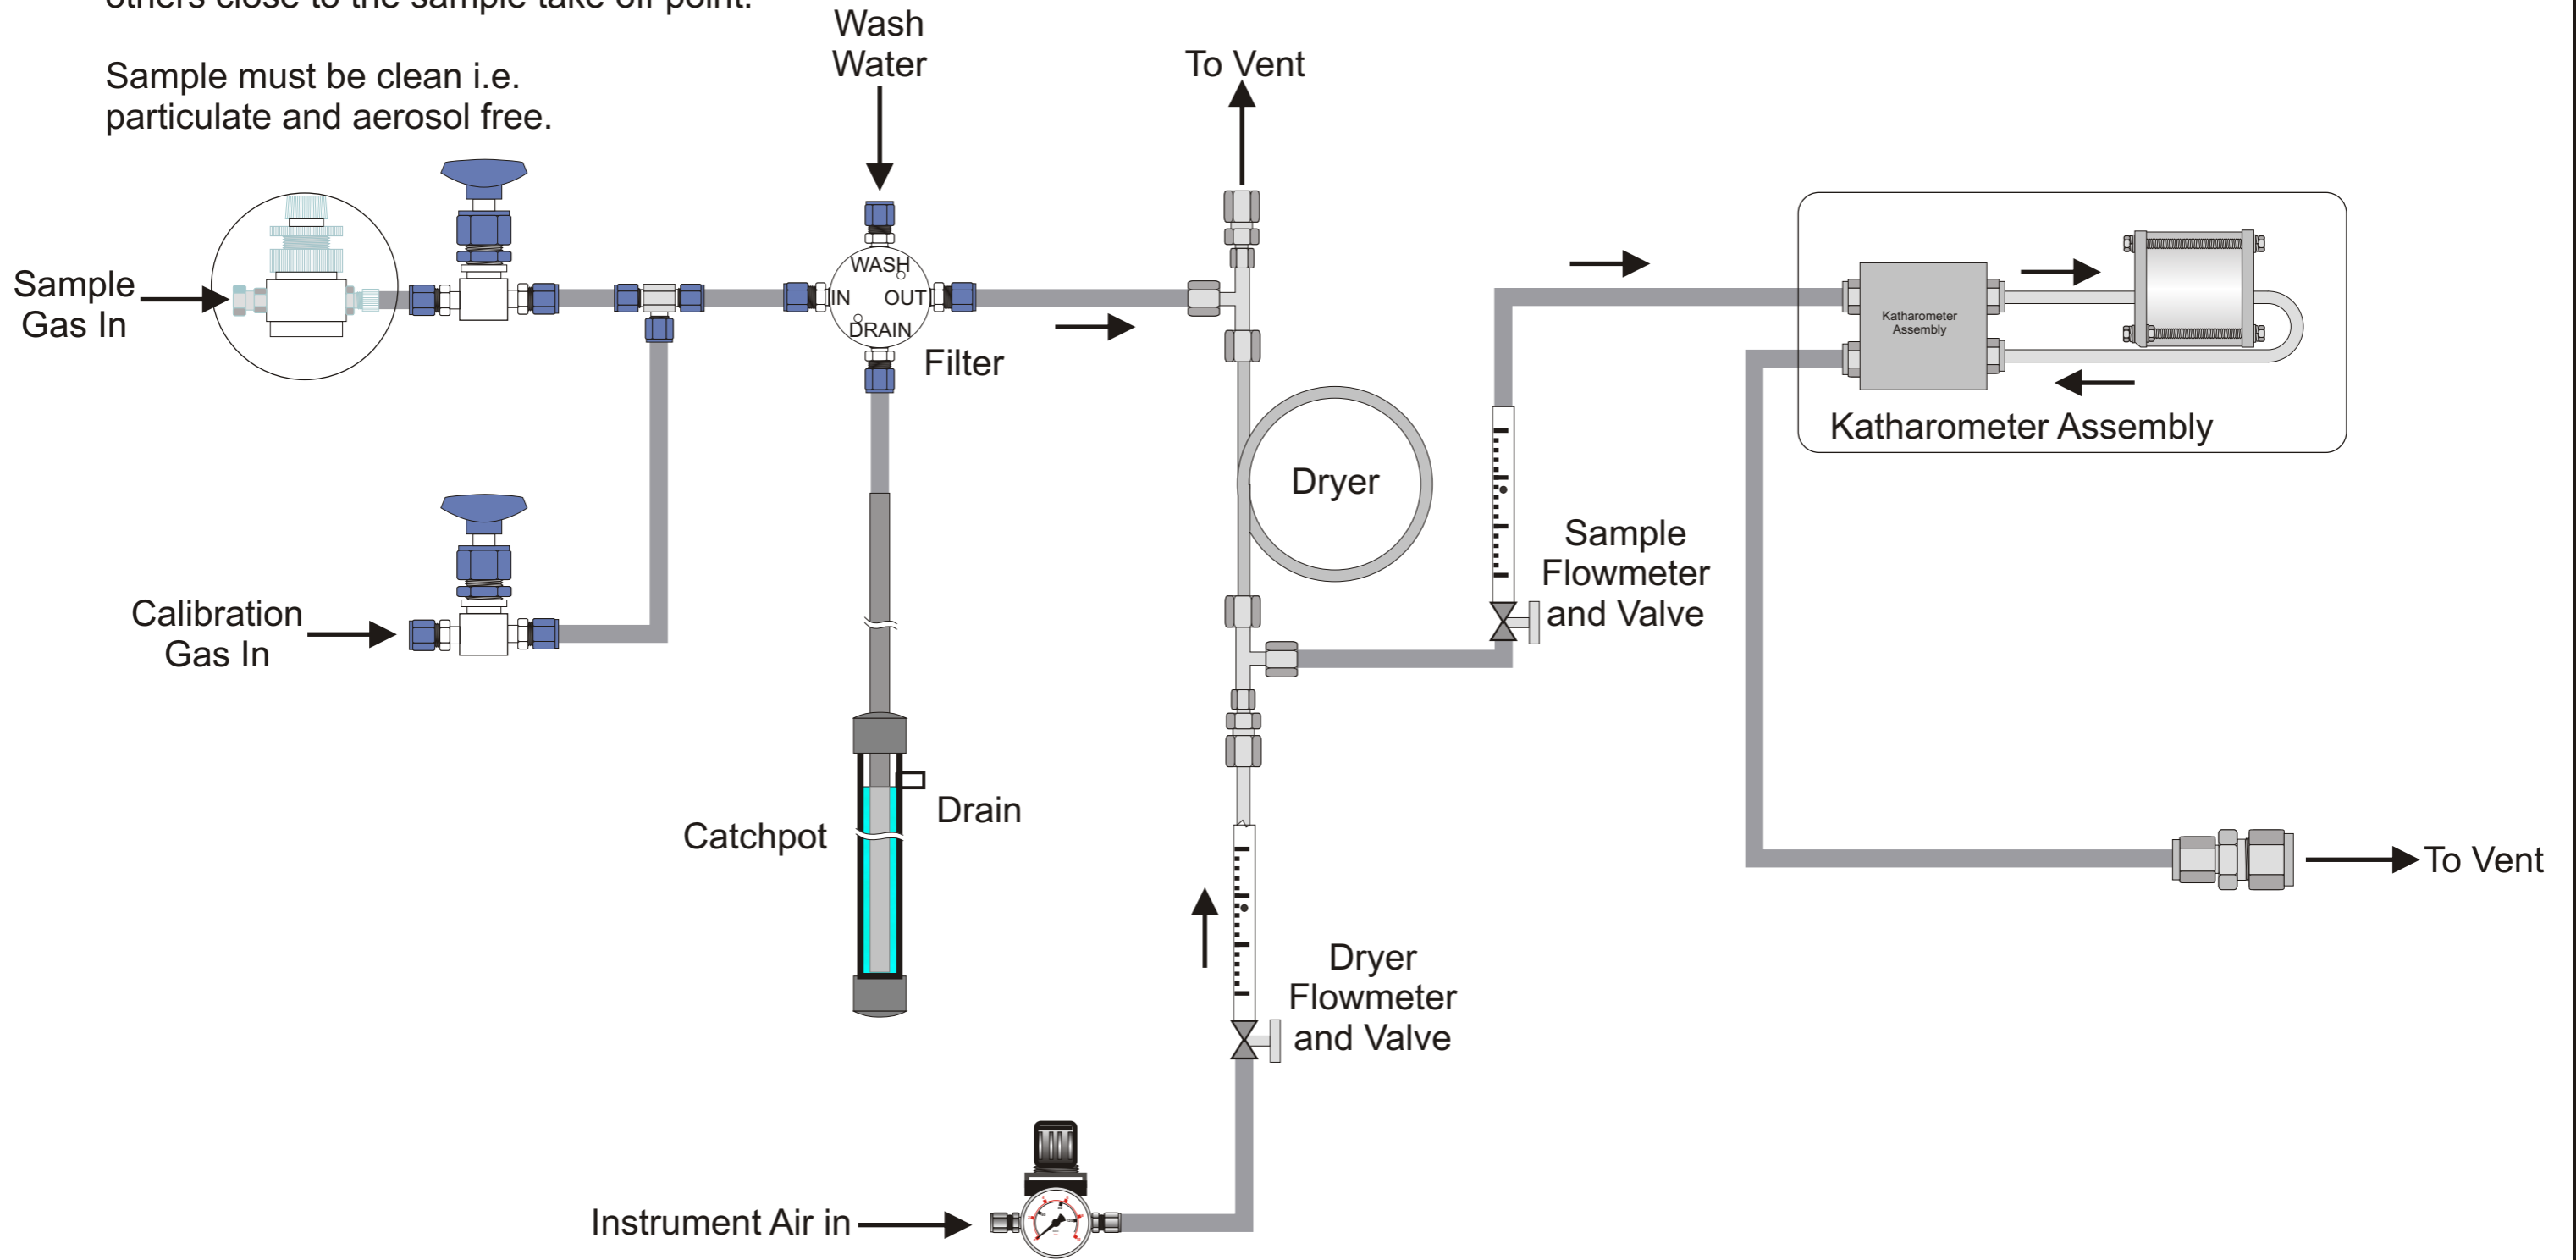

Note: This system is for safe area installation only

Note: This is a schematic drawing only and is issued for information and guidance only

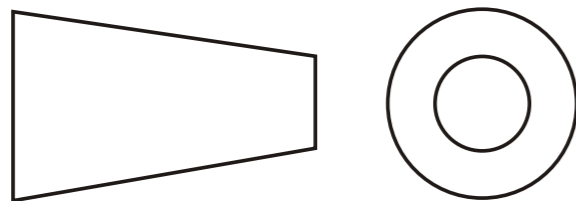

Issue	Description	Date	Eng'd by	Sig	Chk'd by	Sig
a	Draft	8/12/04				
1	Release	5/8/05	KB		IH	
2	ECN3191	10/10/07	PD			
3						

HITECH INSTRUMENTS
 Tolerances:
 Dimensions to one decimal place (0.0) ± 0.1
 Dimensions to two decimal places (0.00) ± 0.025
 All other dimensions ± 0.5 unless otherwise stated.
 T=16pt : L=1.0: Dim=0.4: C= 0.15

Drw No. 131-0053	Sheet: 1 Of: 1
Title: Sample Conditioning System for H2 + Cl2 Analyser - pressure regulated	
Scale: Do not scale	File: 131-0053 .cdr